	Document Number	Revision	Page	Date
	TCP005-2	A0	1 of 1	04-26-2016
<b>PRODUCT DATA SHEET</b>		<b>96 Well Cell Attachment Treated Flat Bottom Tissue Culture Plates</b>		


**1: Material:** Plate: GPPS (General polystyrene)    Colour: Clear

Lid: GPPS (General polystyrene)    Colour: Clear

**2: Related Catalog Numbers:**

VWR EU EAN. No.	VWR NA Cat. No.	Description	Packout Description
734-2327	10861-666	96 Well, Treated for Increased Cell Attachment, Sterilized	1/ Tray, 50/PK, 100/Case

**3: Dimensions (Unit:mm)**

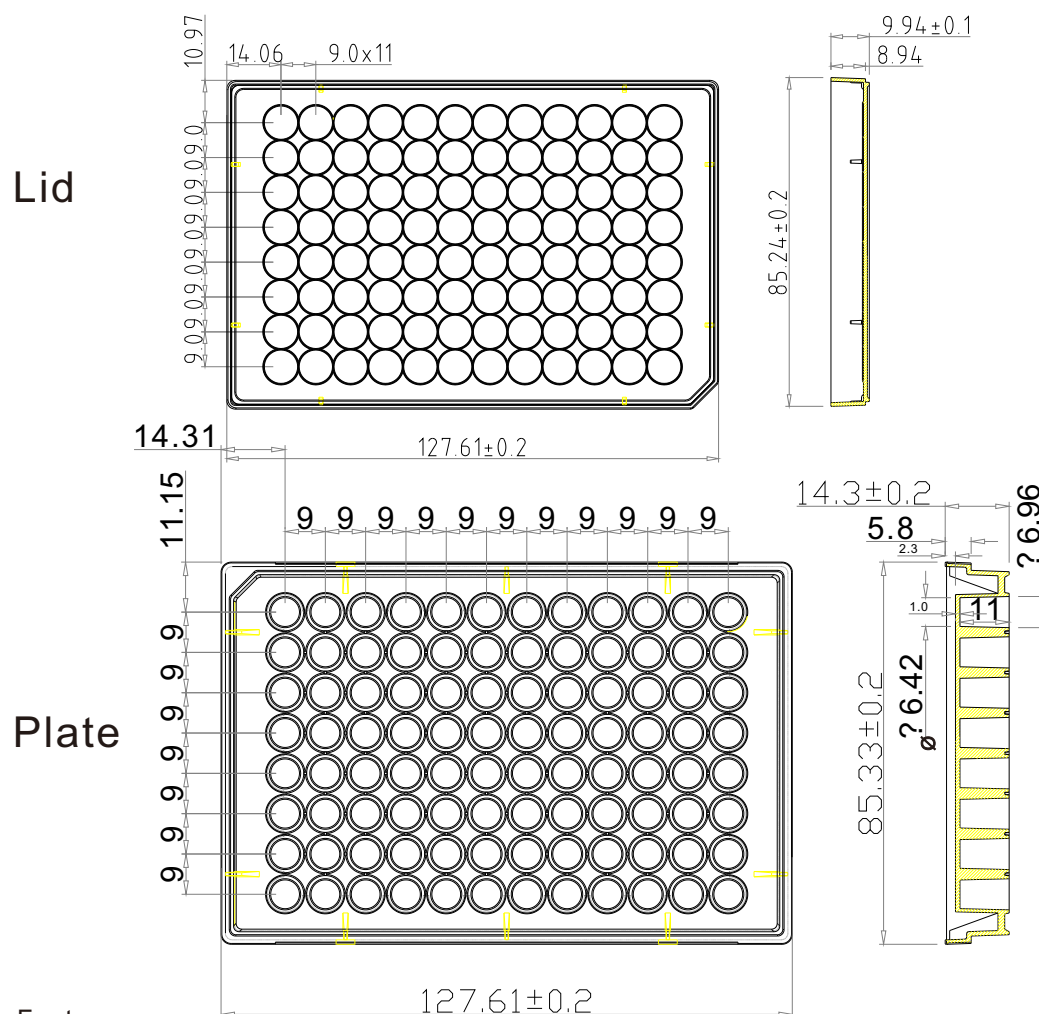

**4: Features:**

- For use in applications where cell attachment is not desired
- Available in individual recyclable PET
- Temperature range: -20°C to +50°C
- Autoclavability: No
- Non-pyrogenic
- Shelf life: 3 years after month of production


**5: STERILITY:**

- Sterilized by gamma irradiation SAL10<sup>-6</sup> (ISO11137)

**6: PRODUCT ISO 9000 CERTIFICATION:**

- Manufactured in a class 100,000 room environment.
- Manufactured under EN ISO13485 :2003 and ISO9001:2008 quality management system.

Drawn	Approved
Date 26 Apr 2016	Date 26 Apr 2016
Name Alex Fang	Name James

	Document Number	Revision	Page	Date
	TCP006-2	A0	1 of 1	04-26-2016
<b>PRODUCT DATA SHEET</b>		<b>96 Well Cell Attachment Treated U-Bottom Tissue Culture Plates</b>		

**1: Material:** Plate: GPPS (General polystyrene)    Colour: Clear


Lid: GPPS (General polystyrene)    Colour: Clear

**2: Related Catalog Numbers:**


VWR EU EAN. No.	VWR NA Cat. No.	Description	Packout Description
734-2328	10861-668	96 Well, U-Bottom, Treated for Increased Cell Attachment, Sterilized	1/ Tray,50/PK, 100/Case

**3: Dimensions (Unit:mm)**

Lid

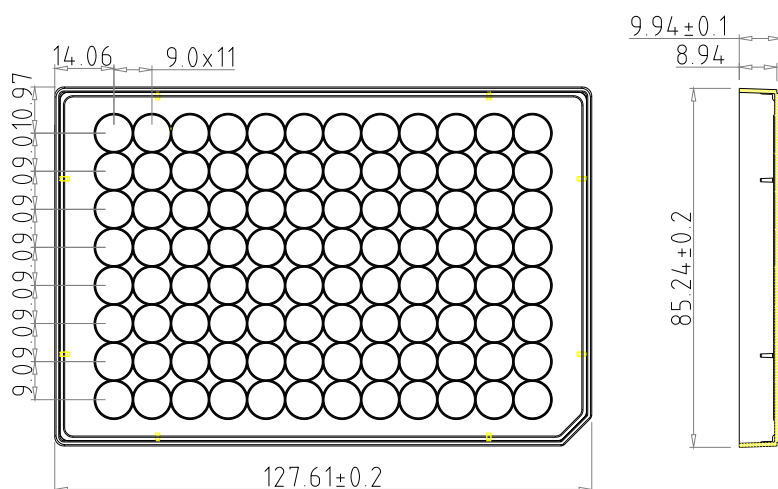

Plate

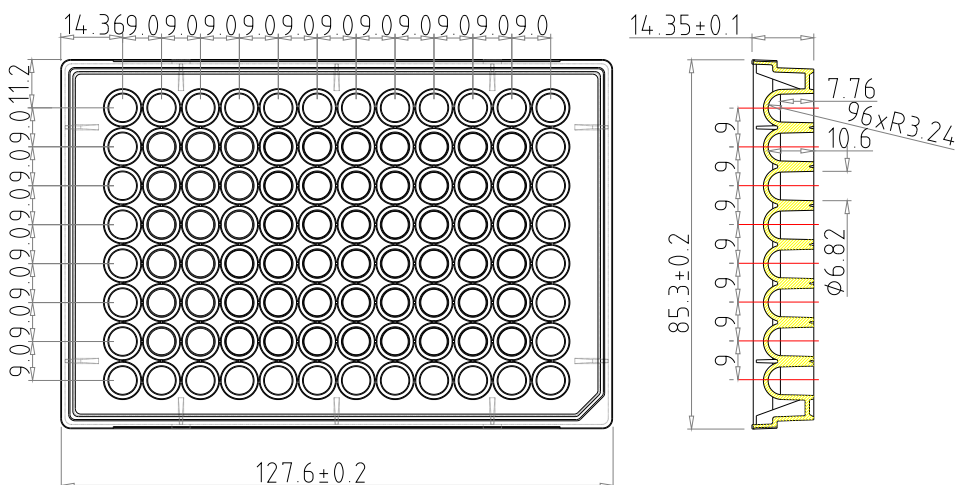

**4: Features:**

- For use in applications where cell attachment is not desired
- Available in individual recyclable PET
- Temperature range: -20°C to +50°C
- Autoclavability: No
- Non-pyrogenic
- Shelf life: 3 years after month of production

**5: STERILITY:**

- Sterilized by gamma irradiation SAL10<sup>-6</sup> (ISO11137)

**6: PRODUCT ISO 9000 CERTIFICATION:**

- Manufactured in a class 100,000 room environment.
- Manufactured under EN ISO13485 :2003 and ISO9001:2008 quality management system.

Drawn	Approved
Date 26 Apr 2016	Date 26 Apr 2016
Name Alex Fang	Name James